

# BODILINK HEAD SUPPORT

## ORDER FORM

Patent Pending



CUSHIONED HEADREST  
REMOVABLE HARDWARE

Company Name/ACCT #: \_\_\_\_\_

P.O. Number: \_\_\_\_\_

Requested By: \_\_\_\_\_

Phone: \_\_\_\_\_ Fax: \_\_\_\_\_

Email: \_\_\_\_\_

Ship To: \_\_\_\_\_

Patient Reference: \_\_\_\_\_

HEAD SUPPORT-LCS-NP-01/04/2017

If you would like an official quotation, please email completed form to [regina@lcseating.ie](mailto:regina@lcseating.ie), or fax to 00353 71 9163918

If you have any queries, please contact the office on 00353 71 9163905



14W x 5L Head Support Pad Pictured

## 1 BODILINK HEAD SUPPORT PAD

### 1.1 HEAD SUPPORT PAD STYLE

Length (L) refers to the actual size dimension of the support from bottom to top edge.

W		Pad Firmness	
L	6W x 3½L	Soft	BL-HSP1-6W3L
		Extra Soft	BL-HSP2-6W3L
L	8W x 4L	Soft	BL-HSP1-8W4L
		Extra Soft	BL-HSP2-8W4L
L	10W x 5L with adjustable wings	Soft	BL-HSP1-10W5L
		Extra Soft	BL-HSP2-10W5L
L	14W x 5L with adjustable wings	Soft	BL-HSP1-14W5L
		Extra Soft	BL-HSP2-14W5L
L	18W x 5L with adjustable wings	Soft	BL-HSP1-18W5L
		Extra Soft	BL-HSP2-18W5L
W			

### 1.2 PAD COVER MATERIAL

<b>GLIDE WEAR.</b>	FOR SKIN PROTECTION & SHEAR REDUCTION. NOT FLUID RESISTANT.
<b>COMFORT-TEK</b>	FOR FLUID PROTECTION & AN EASILY CLEANED SURFACE.
<b>STRETCH-AIR</b>	FOR AIR TRANSMISSION & HEAT DISSIPATION.


	GlideWear® (GLIDEWEAR)
	Comfort-Tek (COMFORT-TEK)
	Stretch-Air (STRETCH-AIR)



All BodiLink Head Support Pads have pre-formed contours. 10W, 14W & 18W Head Support Pads have adjustable wings located approx. 3 inches from the center on each side.

## 2.1


## HEAD SUPPORT HARDWARE

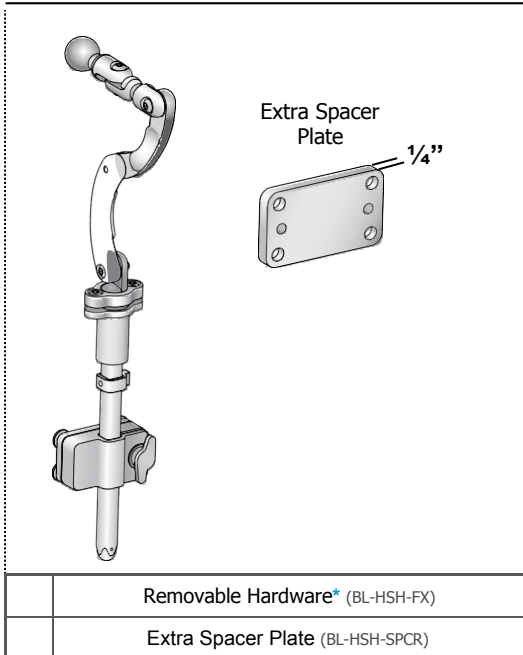

\*Only available for Acta-Relief™ when using COMPASS® POWER MOUNT Hardware. See 2.2 if using COMPASS® 4 hardware.

## 2.2


## FOR ACTA-RELIEF™

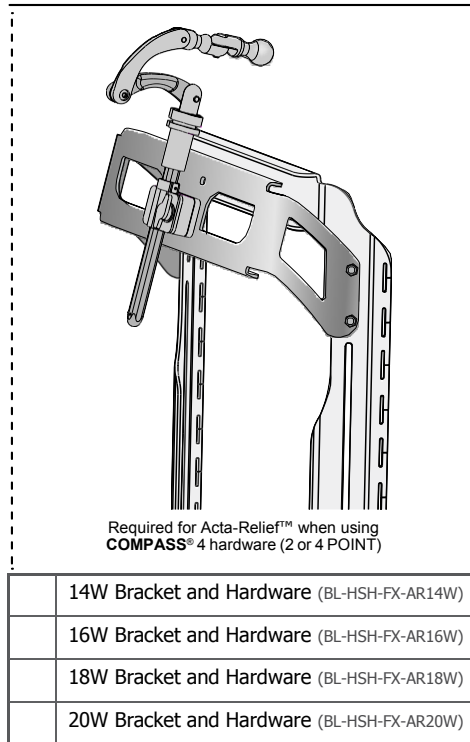

Bodilink Head Support not available for 10"L Acta-Relief™ Back Supports

## 2.3


## \*ADDITIONAL MOUNTING HARDWARE

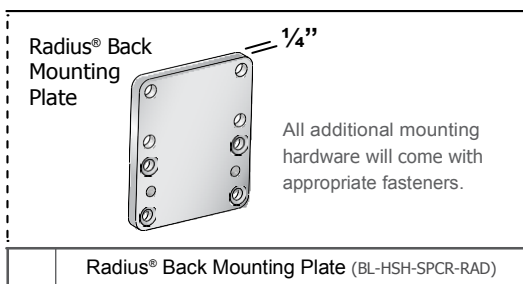

\*Must be ordered in addition to *Removable Hardware* for mounting to the Radius® Back Support.



\*Must be ordered in addition to *Removable Hardware* for mounting to non-Comfort Company back supports from the posterior side, 2" x 1" spacing.



\*Must be ordered in addition to *Removable Hardware* for mounting to Permobil Corpus 3G Uni-Track System.